



SLE 25-017 Laboratory Equipment Sale





SLE 25-017 Laboratory Equipment Sale







SLE 25-017 Laboratory Equipment Sale






SLE 25-017 Laboratory Equipment Sale

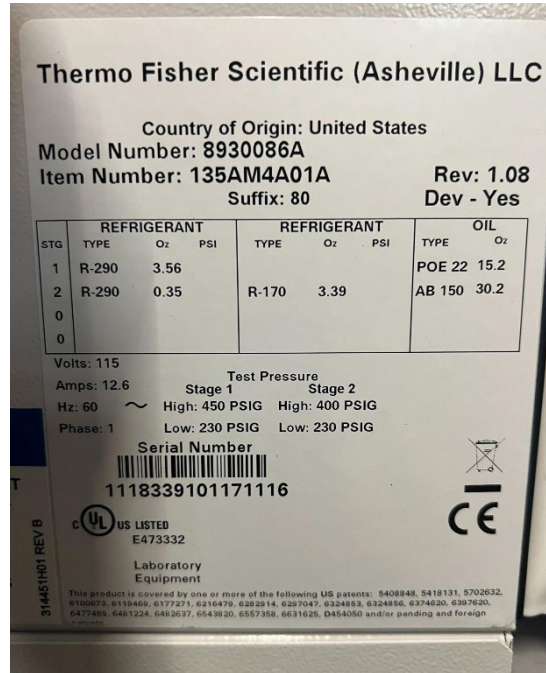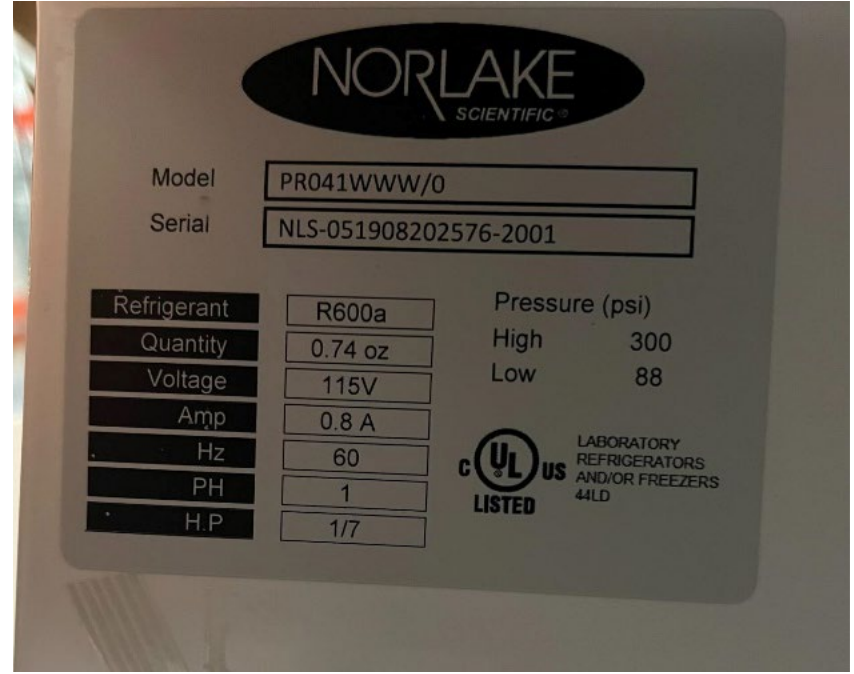




SLE 25-017 Laboratory Equipment Sale

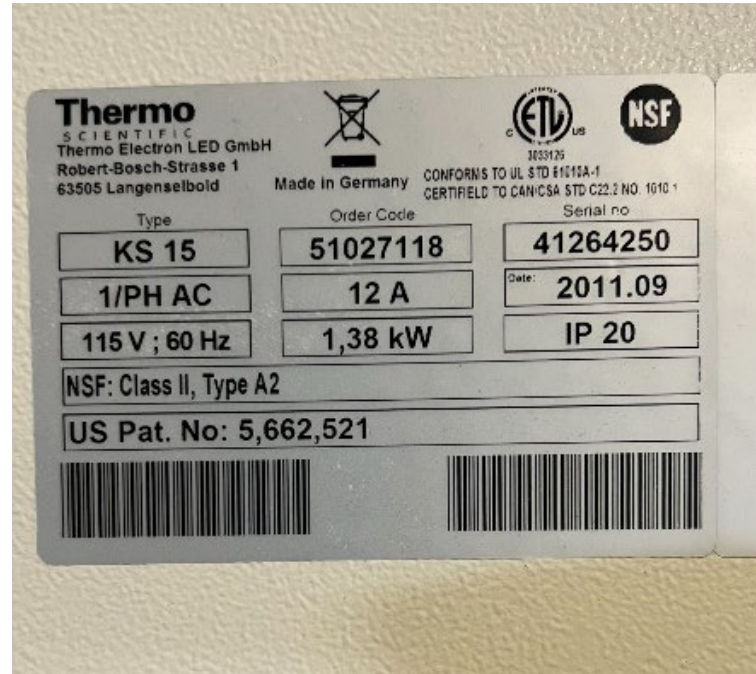



SLE 25-017 Laboratory Equipment Sale

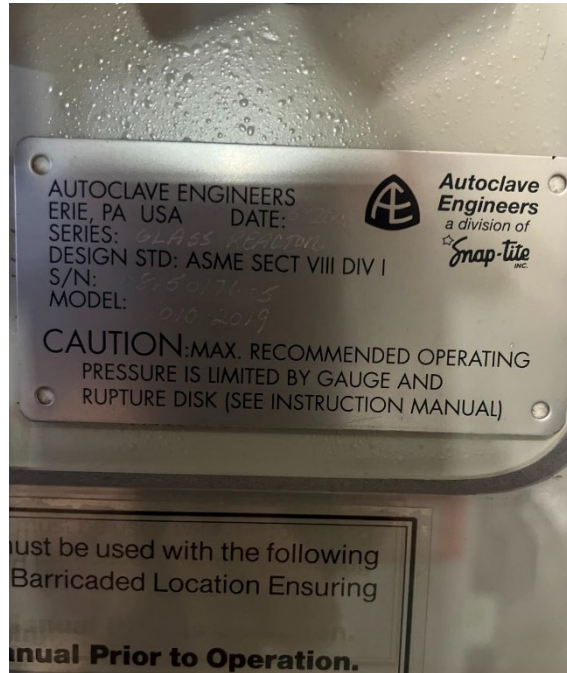



SLE 25-017 Laboratory Equipment Sale





SLE 25-017 Laboratory Equipment Sale



LINDBERG
A UNIT OF GENERAL SIGNAL

MODEL: 54S-M3042-V-5Z-1161 HZ: 50/60
SER.: 98008 MAX. TEMP: 1950 C
VOLTS: 208 WATTS: 5950

LINDBERG PHONE: 800-759-4782
A UNIT OF GENERAL SIGNAL P.O. BOX 3738
304 HART ST. WATERTOWN, WIS.

WARNING
THIS PRODUCT CONTAINS REFRACTORY OR CERAMIC FIBER WHICH MAY CAUSE SEVERE RESPIRATORY IRRITATION. PLEASE USE NIOSH APPROVED RESPIRATORS WHEN MAINTAINING THE REFRACTORY. FOR YOUR PROTECTION YOU MUST READ THE INSTRUCTION MANUAL FOR SAFE MAINTENANCE PROCEDURES.

MANUAL NO. _____

INSTALLATION, OPERATION AND MAINTENANCE INSTRUCTIONS
FOR

TYPE:	54S-M3042-V-5Z-TCH Tube Furnace
SERIAL NO.:	989008 thru 989011 (S.O. 36564)
WIRING DIAGRAM:	7209-1367-00A
OUTLINE OR GENERAL ASSEMBLY:	

INFORMATION CONTAINED HEREIN IS CONFIDENTIAL, IS THE PROPERTY OF GENERAL SIGNAL CORPORATION, IS TO BE USED SOLELY FOR THE PURPOSE PROVIDED, AND IS NOT TO BE DISCLOSED TO OTHERS WITHOUT THE WRITTEN CONSENT OF GENERAL SIGNAL CORPORATION.





SLE 25-017 Laboratory Equipment Sale





SLE 25-017 Laboratory Equipment Sale





SLE 25-017 Laboratory Equipment Sale






SLE 25-017 Laboratory Equipment Sale





SLE 25-017 Laboratory Equipment Sale

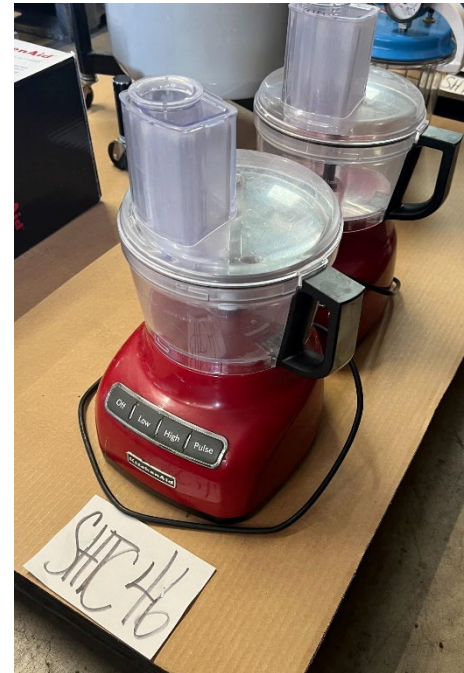




SLE 25-017 Laboratory Equipment Sale





SLE 25-017 Laboratory Equipment Sale

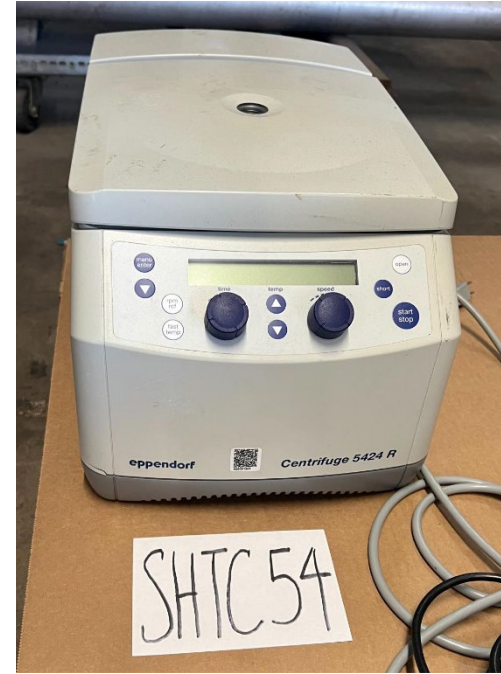



SLE 25-017 Laboratory Equipment Sale





SLE 25-017 Laboratory Equipment Sale





SLE 25-017 Laboratory Equipment Sale






SLE 25-017 Laboratory Equipment Sale





SLE 25-017 Laboratory Equipment Sale

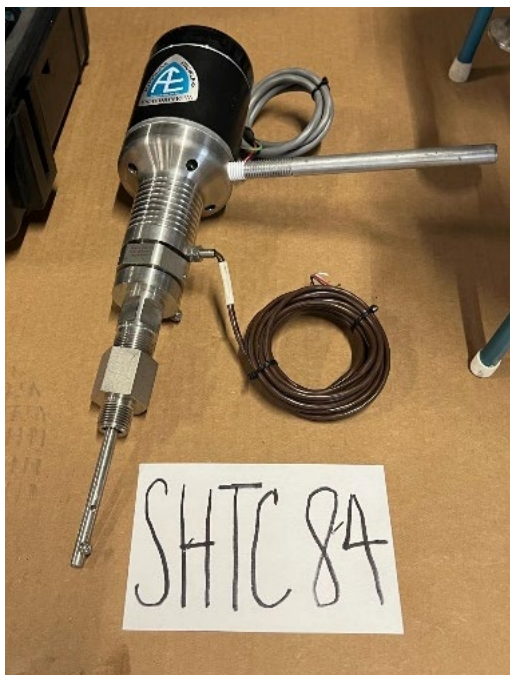




SLE 25-017 Laboratory Equipment Sale





SLE 25-017 Laboratory Equipment Sale

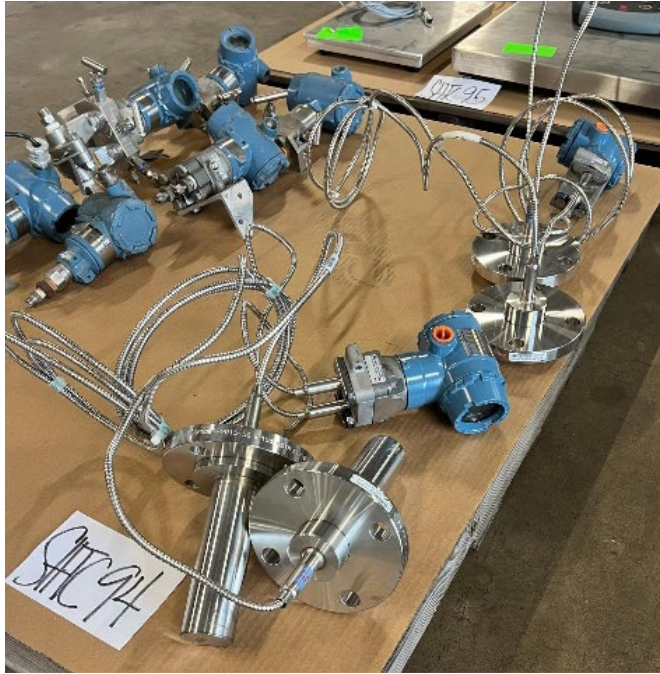



SLE 25-017 Laboratory Equipment Sale

